

AD-A036 669

NATIONAL BUREAU OF STANDARDS WASHINGTON D C INST FO--ETC F/6 9/1
RADIATION-HARDNESS TESTING OF ELECTRONIC DEVICES: A SURVEY OF F--ETC(U)
SEP 76 J C HUMPHREYS, S E CHAPPELL

UNCLASSIFIED

NBSIR-76-1135

NL


| OF |

AD
A036669



END

DATE
FILMED
3-77

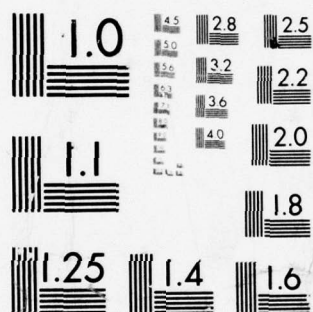

MICROCOPY RESOLUTION TEST CHART
NATIONAL BUREAU OF STANDARDS-1963-A

ADA 036669

NBSIR 76-1135 ✓

(13) 9

Radiation-Hardness Testing of Electronic Devices: A Survey of Facility Dosimetry Practices


J. C. Humphreys and S. E. Chappell

Center for Radiation Research ✓
Institute for Basic Standards ✓
National Bureau of Standards ✓
Washington, D. C. 20234



September 1976

Final

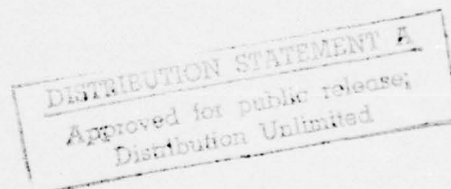

Prepared for
Defense Nuclear Agency
Washington, D. C. 20305
Sponsored Under: Subtask Code Z99QAXD072 and Work Unit 05

401299

13

14

NBSIR-76-1135

2

**RADIATION-HARDNESS TESTING OF
ELECTRONIC DEVICES: A SURVEY
OF FACILITY DOSIMETRY PRACTICES.**

DDC
RECEIVED
MAR 10 1977
C

10

J. C. Humphreys and S. E. Chappell

Center for Radiation Research
Institute for Basic Standards
National Bureau of Standards
Washington, D. C. 20234

| | |
|---------------------------------|---|
| ACCESSION for | |
| NTIS | White Section <input checked="" type="checkbox"/> |
| FC | Buff Section <input type="checkbox"/> |
| UNANNOUNCED | <input type="checkbox"/> |
| JUSTIFICATION | |
| BY | |
| DISTRIBUTION/AVAILABILITY CODES | |
| Dist. | AVAIL. and/or SPECIAL |
| A | |

11

September 1976

12 26p.

9

Final

rept. Jan-Sep 76

Prepared for
Defense Nuclear Agency
Washington, D. C. 20305
Sponsored Under: Subtask Code Z99QAXD072 and Work Unit 05



U.S. DEPARTMENT OF COMMERCE, Elliot L. Richardson, Secretary

Edward O. Vetter, Under Secretary

Dr. Betsy Ancker-Johnson, Assistant Secretary for Science and Technology

NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Acting Director

401299

JB

Table of Contents

| | Page |
|---|------|
| ABSTRACT | 5 |
| 1. INTRODUCTION | 6 |
| 2. FACILITIES VISITED | 6 |
| 3. RADIATION SOURCES | 7 |
| 3.1 Isotope Sources | 7 |
| 3.2 Flash Accelerators | 10 |
| 3.3 Linacs and D.C. Accelerators | 10 |
| 4. CALIBRATION OF THE RADIATION SOURCES | 11 |
| 4.1 γ -Ray Isotope Source Calibration | 11 |
| 4.2 Accelerator Calibration | 13 |
| 5. DOSIMETRY SYSTEMS EMPLOYED DURING DEVICE IRRADIATION | 14 |
| 5.1 Thermoluminescence Dosimeters | 14 |
| 5.2 Dosimeter Calibration | 14 |
| 5.3 Dosimeter Readout Devices | 16 |
| 5.4 Dosimeter Handling Procedures | 17 |
| 5.5 Use of Dosimeters During Device Irradiation | 19 |
| 6. COMMENTS FROM FACILITY PERSONNEL | 19 |
| 7. OBSERVATIONS ON DOSIMETRY PRACTICES | 20 |
| 8. RECOMMENDATIONS | 21 |
| REFERENCES... | 22 |
| APPENDIX | 23 |

List of Tables

| | Page |
|---|------|
| 1. Facilities Visited | 7 |
| 2. Radiation Sources | 9 |
| 3. Dosimeters Used for Calibration of γ -Ray Sources | 12 |
| 4. Thermoluminescence Dosimeters | 15 |
| 5. TLD Readers | 18 |

RADIATION-HARDNESS TESTING OF ELECTRONIC DEVICES:
A SURVEY OF FACILITY DOSIMETRY PRACTICES

J. C. Humphreys and S. E. Chappell


X-Ray Physics Section

Center for Radiation Research

National Bureau of Standards


Washington D.C. 20234

ABSTRACT



As part of a program to develop better quality assurance in the measurement of total dose in the field of radiation-hardness testing of electronic devices, a survey was conducted at twelve radiation test facilities. The survey was carried out through personal visits during which various characteristics of the test facilities and dosimetry procedures were noted. This report summarizes the results of the survey. Particular attention is given to the types of dosimetry problems perceived by the dosimetry personnel at the facilities as well as to general observations by the surveyor.

The observations and information obtained through this survey led to some conclusions on where problems in total-dose measurements may occur. Some specific recommendations result and give direction to the program plan for developing more consistent measurement procedures within the radiation-hardness testing community.



1. INTRODUCTION

At the present time, many different radiation sources and dosimetry systems are used in the radiation-hardness testing of electronic devices and systems, and, in many instances, considerable disagreement and lack of consistency in the experimental results have been observed. This state of affairs has led to confusion and uncertainty about the dosimetry results among users of radiation-hardness testing facilities. Results of an earlier survey on this problem have been reported by D.C. Lewis [1]. In order to help establish more uniform, accurate, and consistent measurements of total dose, the National Bureau of Standards is engaged in a program which is expected to lead to the establishment of reliable dosimetry systems. This survey represents a first step in this program. In this report, the term "total dose" means the energy absorbed per unit mass in a specific material as a result of irradiation by photons or electrons. This report does not address measurements of dose rate resulting from irradiation by photons or electrons, or measurements of dose resulting from neutron irradiation.

2. FACILITIES VISITED

Table 1 lists the facilities visited. Although this is not a comprehensive listing of all facilities of the radiation-hardness testing community, these are considered to be fairly representative.

Throughout the remainder of this report, the observations and conclusions on radiation sources and dosimetry will be based on a compilation of information gathered from all these facilities. The purpose here is to identify the dosimetry practices and problems that may be experienced by the radiation-hardness testing community in general. Therefore, no attempt will be made to identify the dosimetry practices of a particular facility. A checklist of the type of information sought at each facility is given in the Appendix.

TABLE 1

Facilities Visited

| <u>Facility</u> | <u>Location</u> |
|-------------------------------------|-------------------------|
| Air Force Weapons Laboratory | Albuquerque, New Mexico |
| White Sands Missile Range | New Mexico |
| Harry Diamond Laboratories | Adelphi, Maryland |
| Naval Surface Weapons Center | White Oak, Maryland |
| Jet Propulsion Laboratory | Pasadena, California |
| Sandia Laboratories | Albuquerque, New Mexico |
| Boeing Radiation Effects Laboratory | Seattle, Washington |
| Hughes Aircraft | Los Angeles, California |
| IRT Corporation | San Diego, California |
| Northrop Corporation | Los Angeles, California |
| Rockwell International | Los Angeles, California |
| TRW Systems Group | Los Angeles, California |

3. RADIATION SOURCES

A variety of radiation sources was seen at the facilities visited. These sources ranged from low-activity γ -ray isotope sources to the very large flash accelerators. Table 2 gives a summary of the number of various kinds of sources observed and, where applicable, the basis of calibration of the sources. Some of the ^{60}Co and ^{137}Cs sources were used only for dosimeter calibration while others were used for both dosimeter calibration and electronic device irradiation. In general, the accelerators of all types were used only for irradiation of electronic devices and systems.

3.1 Isotope Sources

The isotope γ -ray sources (^{60}Co or ^{137}Cs) observed can be grouped into four basic geometry categories:

- (1) lead-shielded well irradiator, with the specimen to be irradiated placed inside a cylindrical array of source tubes;
- (2) collimated-beam irradiator, with the irradiated specimen in air on the axis of a beam port in the lead housing that shields the source;

TABLE 2

Radiation Sources

| Type | Total Number | Number of Calibrated Sources | Calibration Instrument Used | |
|--|--------------|------------------------------|-----------------------------------|---------------------------------|
| | | | Type | For Specified Number of Sources |
| ^{60}Co γ -Ray Source | 20 | 21 | Ion Chamber | 18 |
| | | | TLD and ion chamber | 2 |
| ^{137}Cs γ -Ray Source | 3 | | Fricke* dosimeter and ion chamber | 1 |
| | | | Calorimeter | 4 |
| Flash Accelerator | 13 | 4 | Calorimeter | 2 |
| | | | Fricke* dosimeter | 1 |
| Linac | 4 | 3 | Calorimeter | 1 |
| | | | Fricke* dosimeter | 1 |
| D.C. Accelerator | 3 | 2 | Calorimeter | 1 |
| | | | Faraday cup | 1 |

*ferrous sulfate

(3) open-air source, with the irradiated specimen either in the center or to one side of a cylindrical or planar array of sources; and

(4) pool source, which is usually a cylindrical array of sources at the bottom of a water well, with the specimen placed in the center of the array inside a watertight can.

The γ -ray spectrum from a particular isotope source varies depending upon the specific activity of the source, the details of the source encapsulation, and the material surrounding the source capsule. Some general comments can be made, however, about the various source geometries described above. The lead-shielded well-type irradiators will have more low-energy scattered photons in their spectrum than the other three types; the open-air source geometry usually has the "cleanest" spectrum. Because of the scatter introduced by shielding materials, source capsules, etc., knowledge of the scattered photon energy spectrum is an important parameter. This is because a dosimeter or device whose radiation response is energy dependent will be affected differently by equal exposures with a source having a "dirty" spectrum than with a "clean" source. Therefore, errors can be introduced in the source calibration as well as in the use of the source for dosimeter calibration and device irradiation if the photon energy spectrum of the source is not taken into account. In only one of the 12 facilities visited was any knowledge expressed of the energy spectra of the isotope sources used. The activities of the isotope sources seen ranged from 50 Ci to 50 kCi, with corresponding maximum dose rates of 100 rad/h to 8 Mrad/h in silicon. In this report, the quantity, absorbed dose in silicon in units of rads or kilorads, will be abbreviated as rad (Si) or krad (Si).*

*The International Committee of Weights and Measures (CIPM) has recently adopted new special names for SI units in the field of ionizing radiations. The SI unit for absorbed dose, the joule per kilogram, is called the gray with the symbol Gy; $1 \text{ Gy} = 100 \text{ rad} = \text{J kg}^{-1}$. The SI unit for activity, the reciprocal second (one per second), is called the becquerel, symbol Bq; $1 \text{ Bq} = 1 \text{ s}^{-1} \approx 2.703 \times 10^{-11} \text{ Ci}$ [2].

3.2 Flash Accelerators

The fast-pulse (flash) accelerators used at the facilities visited have maximum electron-beam energies varying from about 0.8 MeV for the smaller machines up to 12 MeV for the largest machines. These machines are used primarily in the x-ray (bremsstrahlung) mode; only a few utilize the primary electron beam for irradiations. Generally, in the x-ray mode, the maximum deliverable total dose per pulse to a specimen is about 10 krad (Si) for the lower output machines up to about 100 krad (Si) for the higher output machines. Maximum dose rates available in the x-ray mode are of the order of 10^{11} - 10^{12} rad (Si)/s. The facilities use either PIN diodes or scintillator-photodiodes, or both, as photon-beam monitors for every irradiation pulse. None of the facilities reported detailed knowledge of the bremsstrahlung energy spectra mainly because of the difficulty involved in making direct spectral measurements during the fast output pulse (typically 100 ns full width at half maximum). Several facilities do have approximations of the available photon energy spectra derived from calculations and indirect measurements.

3.3 Linacs and D.C. Accelerators

The linacs observed ranged from a single-section machine (10-MeV maximum electron energy), to a four-section machine (60-MeV maximum energy). Most of the multisection machines are used with a varying number of accelerating sections to give several different electron-beam energy and current combinations. All of the linacs are used primarily in the electron-beam mode although most are readily convertible to the x-ray mode with the addition of a bremsstrahlung converter. With direct electron beams, the linacs can give doses per pulse from less than one rad (Si) up to 100 krad (Si). Dose rates up to about 10^{11} rad (Si)/s can be obtained. Beam monitors used are PIN diodes and secondary-electron emission devices.

In addition to the linacs, three d.c. accelerators were observed. The maximum electron energy is 1 MeV for one of these and 2.5 MeV for the other two machines. Two of the machines use electron beams only

while the other machine is used either in an electron or a positive-ion acceleration mode. The dose rates available from electron beams are in the range of 10^6 - 10^9 rad (Si)/s. Most of the time, a Faraday cup is used as a beam monitor on these d.c. accelerators.

4. CALIBRATION OF THE RADIATION SOURCES

In order to make measurements of the effects of irradiation on an electronic device, it is necessary to calibrate the output of the radiation source. At the facilities surveyed, the methods of source-output calibration fall into two general categories: those used for γ -ray isotope sources and those used for accelerators (flash, linac, or d.c.). See Table 2 for a summary of the methods.

4.1 γ -Ray Isotope Source Calibration

Nearly all of the facilities visited used air-ionization chambers as the primary method of γ -ray source-output calibration. In some facilities, these chambers were used in conjunction with other dosimeters. Only three of the sources were calibrated by other methods: one by a Fricke (ferrous sulfate) system, and two others by a TLD ($\text{CaF}_2\text{:Mn}$) system that had been calibrated at another source which, in turn, had been calibrated with an ion chamber. Table 3 gives details on the instruments used for source calibrations. Of the ion chambers used, 75 percent had been periodically calibrated at NBS, and the remainder had been calibrated by their manufacturer. The frequency of source calibration varied from one to four years. Most of the facilities have had their ion chambers recalibrated at one-to-two year intervals. The quantity usually measured by an air-ionization chamber irradiated by photons is exposure in units of roentgens (R). For radiation-hardness testing of electronic devices, the quantity of interest is dose in units of rads in silicon (rad (Si)). Therefore, a conversion factor is necessary to convert exposure (R) to dose (rad (Si)).

TABLE 3

Dosimeters used for Calibration of γ -ray Sources

| <u>Number of Sources</u> | <u>Model of Ionization Chamber*</u> | <u>Other type of Dosimeter</u> |
|------------------------------|---|------------------------------------|
| 6 | Landsverk L-64 | none |
| 4 | Victoreen 570 | none |
| 3 | EG&G IC-17 | none |
| 2 | Landsverk L-64 + EG&G IC-17 | none |
| 1 | Farmer 2505 | none |
| 2 | NRL graphite + EG&G IC-17 | none |
| 1 | Victoreen 570 | Fricke dosimeter |
| 2 | EG&G IC-17 | TLD ($\text{CaF}_2\text{:Mn}$) |

*Throughout this report, the identity of the manufacturer or type of dosimeters and other equipment is revealed in order to make explicit the results of this survey. It does not in anyway imply an endorsement or recommendation by the NBS.

4.2 Accelerator Calibration

As can be seen from Table 2, the radiation output from the flash accelerators has been calibrated in only a few cases. Calorimeters of various types were used to measure the output of the four calibrated machines. The characteristics of these calorimeters were as follows:

(1) Four designs employed thin foils of materials such as C, Al, Ta, and Au. One design used a single foil, and the rest employed multiple stacks of foils. Foil thicknesses were of the order of 25 to 100 μm .

(2) Four designs used thick C or Al elements to totally absorb the irradiation beam.

(3) Two designs utilized single silicon wafers with dimensions of about 3 x 3 mm by 250 μm thick.

(4) Generally, the associated temperature sensors were thermocouples soldered or welded to the foils or the silicon wafers; however, a few employed thermistors which permitted measurements at lower dose levels.

(5) One design consisted of a spherical silicon core surrounded by a hollow spherical silicon shield and employed a thermistor temperature sensor in the core [3]. In this case, the spherical geometry eliminated directional effects on the calorimeter response for nonplanar photon beams.

In most facilities using electron beams from the linacs and d.c. accelerators, the beam output was calibrated by means of calorimeters similar to those employed for the flash x-ray machines. However, in one case, a Fricke (ferrous sulfate) dosimeter system was employed to calibrate both the electron and x-ray beams from a linac, and, in another instance, the electron beam from a d.c. accelerator was characterized by the charge collected with a Faraday cup in vacuum.

5. DOSIMETRY SYSTEMS EMPLOYED DURING DEVICE IRRADIATION

As had been expected, the survey revealed that thermoluminescence dosimetry (TLD) is employed by nearly all of the facilities as the principal method of dosimetry for electronic-device irradiations. A few facilities occasionally employ other methods, such as cobalt glass and plastic dye films, but these are generally used only to supplement TLD measurements.

5.1. Thermoluminescence Dosimeters

The TLDs utilized by the facilities visited are shown in Table 4. They are listed by manufacturer, type, physical form, and the number of facilities that used the specific physical form listed. The most commonly used type was $\text{CaF}_2\text{:Mn}$ which was seen in a total of 13 systems in five physical forms. The next most popular was LiF in six systems and in four forms. $\text{Li}_2\text{B}_4\text{O}_7\text{:Mn}$ was employed in a single system and form. Most facilities used only one, or at most two, types of TLDs, with only two facilities using as many as three types.

5.2 Dosimeter Calibration

All facilities visited calibrated their TLDs with γ rays from either ^{60}Co or ^{137}Cs sources. The calibration procedures varied greatly from facility to facility. In some cases, where relatively few dosimeters were used in a given time period, each dosimeter was calibrated and given an identity that was maintained throughout its useful life. In other cases, where TLDs were used in large quantities (e.g., as many as 15 000 per year), only a few dosimeters from each batch were selected and calibrated to obtain a calibration factor which characterized the entire batch. Most facilities used the batch-calibration procedure with batch sizes varying from 1000 to 15 000. In one facility, all new batches were 100 percent screened initially to eliminate any "mavericks," i.e., dosimeters whose responses deviated significantly from the batch average. This facility used $\text{CaF}_2\text{:Mn}$ in the form of solid rods with

TABLE 4

Thermoluminescence Dosimeters

| <u>Manufacturer</u> | <u>Type</u> | <u>Physical Form</u> | <u>No. of Facilities Using Specified Form</u> |
|---------------------|---|---|---|
| Teledyne | CaF ₂ :Mn | Pressed chips | 1 |
| | | Teflon discs | 3 |
| | LiF | Teflon discs | 2 |
| | | Teflon rods | 1 |
| | Li ₂ B ₄ O ₇ :Mn | Teflon discs | 1 |
| EG&G | CaF ₂ :Mn | Pressed chips in bulbs | 2 |
| | | Pressed chips | 1 |
| | | Powder in glass tubes | 1 |
| | LiF | Powder in glass tubes | 1 |
| Harshaw | CaF ₂ :Mn | Pressed chips | 4 |
| | | Square rods | 1 |
| | LiF | Loose powder in thick Teflon capsule | 1 |
| | | Loose powder in thin gelatin capsule | 1 |

square cross sections and annealed the dosimeters after each irradiation and readout.

Typically, most facilities generate a calibration curve that covers a dose range of about 1 rad to about 200 krad with the dose generally specified in silicon or in the TLD material. This curve characterizes an entire batch, or, in some cases, all batches of the same TLD type and manufacturer. Subsequent batches generally are checked at only one dose (e.g., 2 krad (Si)), in order to obtain the calibration factor for this entire new batch. In some cases, different types or forms of TLDs were used for different dose ranges. For example, $\text{CaF}_2\text{:Mn}$ chips were used to cover the range of 0.05 to 10 rad (Si), and LiF-in-Teflon discs from 1 rad to 50 krad (Si).

The geometrical arrangements of the TLDs with respect to the γ -ray source during calibration irradiations varied among the facilities. In about half the cases, material of sufficient thickness to achieve electron equilibrium conditions surrounded the sensitive elements of the dosimeters during irradiation. This material generally was Lucite or aluminum. However, in some cases, Lucite or other plastic material whose thickness was only 20 percent (or less) of the thickness required for equilibrium conditions encased the dosimeters.

In a number of facilities, the dosimeters were discarded after a single irradiation. Generally, this was the procedure for the TLD forms consisting of the TL phosphor powder uniformly distributed in a Teflon matrix. Most facilities that used $\text{CaF}_2\text{:Mn}$ in solid or powder forms, and a few that used LiF powder, annealed the dosimeters after irradiation and readout for reuse. The annealing procedure varied greatly among the facilities. Those using LiF powder and some employing $\text{CaF}_2\text{:Mn}$ used carefully timed and well-controlled heating and cooling cycles while others were quite casual about the time-temperature cycle during annealing.

5.3 Dosimeter Readout Devices

The reader is an integral part of a TLD system. Therefore, its characteristics and performance with a given TLD must be well under-

stood. The manufacturer and model of the various TLD readers seen at the facilities visited are shown in Table 5, along with the types of TLDs that were read out with a given model. A given reader generally was used to read out only one or two types or forms of TLDs. All the readers, except for one model, produced an output that indicated the integral light sum from a TLD. The exception, the EG&G units, indicated the peak light output from a dosimeter on a built-in chart recorder. A majority of the readers used a factory preset heating cycle appropriate for a particular TLD. However, several facilities have adjusted or modified their readers to give heating cycles which, the facility staff felt, produced more reliable data. The heating cycles varied with reader models, their modification, and type of TLD. Some used linear heating ramps while others brought the TLDs quickly up to a constant temperature for readout. All of the readers are equipped with some type of check light source to enable the operator to verify that the instrument is operating in a stable and reproducible manner. At most of the facilities, the check light sources were used at the beginning of the day (or TLD batch) and then again at intervals of a few minutes to several hours.

5.4 Dosimeter Handling Procedures

Observations of dosimeter handling procedure and environmental conditions during irradiation and readout were made at all facilities. In all cases, bare TLDs were handled either with tweezers or, in two facilities, with vacuum-pickup probes. None of the facilities consciously attempted to shield the dosimeters from exposure to UV light from either fluorescent lamps or sunlight. In nearly half of the laboratories, dry nitrogen gas was flowed over the TLDs during readout. Some of the other facilities used readers that had no provision for using inert gas during readout. The elapsed time between irradiation and readout varied widely. In most cases, elapsed times varied from five minutes to a few hours. None of the facilities using LiF or $\text{Li}_2\text{B}_4\text{O}_7$ and only a few of those using CaF_2 TLDs kept an accurate record of elapsed time; consequently, most facilities made no attempt

TABLE 5

TLD Readers

| <u>Manufacturer</u> | <u>Model</u> | <u>No. of facilities using specified reader model</u> | <u>TLD Types</u> | <u>No. of facilities using specified TLD type</u> |
|---------------------------|--------------|---|---|---|
| Harshaw | 2000 | 6 | CaF ₂ :Mn | 6 |
| | | | LiF | 1 |
| Teledyne | 7300 | 4 | CaF ₂ :Mn | 3 |
| | | | LiF | 3 |
| | | | Li ₂ B ₄ O ₇ :Mn | 1 |
| Con-Rad (now Teledyne) | 7100 | 1 | LiF | 1 |
| EG&G | TL-3* | 4 | CaF ₂ :Mn | 4 |
| | | | LiF | 1 |
| Eberline | TLR-5 | 1 | CaF ₂ :Mn | 1 |

*This model now manufactured by Victoreen.

to correct for fading of the TLD response. One facility waited overnight to read all of their CaF_2 TLDs in order to minimize errors associated with fading effects. However, in two labs the elapsed time was accurately measured, and a fading-correction factor was applied to each CaF_2 dosimeter reading.

5.5 Use of Dosimeters During Device Irradiation

The TLDs were arranged in a variety of geometrical configurations when they served as radiation monitors during irradiation of electronic components or systems. Two of the most commonly employed configurations are discussed here. One method was to place essentially bare dosimeters (i.e., TLDs that were neither encapsulated nor encased in material thick enough to produce electron equilibrium conditions) next to, or in front of, the electronic devices being tested. Sometimes these dosimeters were held in place by thin gelatin capsules or similar material. Irradiation of this configuration supposedly would produce approximately the same absorbed dose in the TLDs as in the device. In another arrangement, the TLDs, located inside equilibrium build-up material of Lucite, aluminum, tantalum, or combinations of these and other materials, were placed in the vicinity of the devices being tested. This latter arrangement supposedly made possible a prediction of the absorbed dose in silicon per unit incident photon fluence under equilibrium conditions as a result of irradiation by the particular radiation source used. Some of the facilities made measurements in both configurations. Most of the dosimeters were used to measure doses up to about 100 krad (Si) with only a few being exposed to higher dose levels.

6. COMMENTS FROM FACILITY PERSONNEL

A significant number of the facility staff interviewed expressed some dissatisfaction with their TLDs or readers and sometimes with both. Several mentioned that from five to ten percent of a large batch of TLDs gave responses as much as 50 percent different from the rest of the batch. This was true especially for the TLDs in a Teflon

matrix, where the problem was thought to be caused by a non-uniformity of the TL powder-Teflon mixture. This same type of dosimeters also produced erratic readout results in some types of readers, apparently because of poor thermal contact with the heating planchet. Another difficulty observed with the Teflon-matrix type of TLD was the production of a greasy residue if the TLD was overheated during the readout cycle. When this occurred the residue was deposited on the optical surfaces in the reader and reduced the light received by the photomultiplier tube. Other difficulties mentioned include electronic instabilities in the readers in the form of drifts and sudden shifts in sensitivity or in temperature readings. As might be expected, facilities with heavy work schedules have had problems with mechanical and electrical failures of their TLD readers. When asked about the overall accuracy and reproducibility of their dosimetry measurements, some facility personnel did not attempt to estimate an overall accuracy, but felt that their reproducibility was about 5-10 percent. Others stated an accuracy and a reproducibility of about 10 percent.

7. OBSERVATIONS ON DOSIMETRY PRACTICES

A number of practices were observed during the survey that could have adverse effects on the reproducibility and/or the accuracy of the dosimetry results. These are summarized as follows:

(1) Lack of sufficient equilibrium build-up material around the TLDs, either during calibration (by γ -ray sources) or during irradiation (by flash x-ray beams). This may not be a serious problem in all cases, but the magnitude of this effect should be experimentally verified.

(2) Possible incorrect conversion from exposure (in roentgens) to absorbed dose (in rads) in the material of interest.

(3) Inadequate annealing techniques of TLDs such as poor temperature control of the annealing oven, erratic annealing periods, annealing periods that were too short, and erratic cooling rates.

(4) Poor control of heating and cooling rates during TLD readout caused either by erratic reader performance, or by inconsistent dosimeter-handling techniques during readout, or both.

(5) Lack of attention to elapsed time between irradiation and readout of TLDs with resultant lack of correction for fading of the response.

(6) Neglect of possible need for correction for nonlinearity of the TLD response at high doses.

(7) Exposure to UV light that can cause spurious responses or enhanced fading of TLDs (particularly $\text{CaF}_2\text{:Mn}$) used for low dose measurements.

8. RECOMMENDATIONS

Guidance is needed for workers in the radiation-hardness testing community on how to eliminate difficulties and inconsistencies in the measurement practices and procedures used for determining total dose. It has been decided that an efficient and effective way to do this would be through the voluntary consensus standards process in ASTM. With this goal in mind, work is underway to prepare (1) guidelines on how to use presently available TLD systems effectively, and (2) guidelines on how to calibrate photon sources which in turn are used to calibrate TLDs. In addition, plans are being made to study, on a pilot basis, the feasibility of developing a measurement-assurance program for the radiation-hardness testing facilities.

An approach needs to be developed to solve the "maverick" dosimeter problem. One possibility would be to obtain better quality control of both TLDs and their readers from the manufacturers of these products. This is of particular importance to facilities in which the TLDs are used only once and then discarded. Another possible solution would be the development of a simple 100 percent screening technique for large TLD batches. One possible configuration of such a screening technique would involve the calibration of every TLD in a batch and reuse only those found to have suitable responses. Still another alternative would be to avoid using the types of TLDs that have a "maverick" problem. Appropriate attention also should be given to developing automated handling-readout systems to the maximum extent possible for users of large quantities of TLDs.

REFERENCES

- [1] Lewis, David C., "The Status of Dosimetry used for Studies of the Effects of Radiation on Electronic Devices and Systems," presented at the IEEE Annual Conference on Nuclear and Space Radiation Effects, Arcata, CA, July, 1975 (unpublished).
- [2] Linden, K., "The New Special Names of SI Units in the Field of Ionizing Radiations," Phys. Med. Biol., 20, 1029, 1975.
- [3] Murray, K. M., "An Absolute Silicon-Dose Calorimeter," Nuc. Inst. Meth., 107, 109, 1973.

APPENDIX

Checklist of Questions asked in this Survey

- A. Name of test facility; mailing address.
 - 1. Personnel contacted, phone number, their area of responsibility.
- B. Radiation facility: characteristics.
 - 1. Photons: γ -ray sources, make and model, if commercially made.
 - a. Physical surrounding of source during use (in lead or tungsten pig, open air, water).
 - b. Total activity of source.
 - c. Specific activity of source.
 - d. Geometry of source during use.
 - e. How are irradiations timed (including transit times).
 - f. Spectrum of source, if known.
 - 2. Photons: x rays (bremsstrahlung) from linac, flash machine, other accelerator. Make and model of machine.
 - a. Energy of incident electron beam.
 - b. Spectrum of incident electron beam.
 - c. Material and thickness of x-ray converter target.
 - d. Spectrum of incident photon beam.
 - e. Pulse rate of beam.
 - f. Pulse width of beam.
 - g. Beam current (average, peak).
 - 3. Electrons: linac, flash, other. Give make and model.
 - a. Energy of incident beam.
 - b. Spectrum of incident beam.
 - c. Pulse rate of beam.
 - d. Pulse width of beam.
 - e. If scattering foil is used, give material and thickness.
 - f. Beam current (average, peak).
- C. Electronic devices or system being tested; give general description.
 - 1. Location in radiation field.
 - 2. General composition; high- or low-Z materials and their general location in box.
 - 3. General dimensions of system.

D. Dosimetry employed.

1. Calibration of the radiation source.
 - a. Person or organization that performed the calibration.
 - b. Date of this calibration; the frequency with which the calibration is performed.
 - c. Type of dosimeter(s) used; manufacturer.
 - d. If calibration of dosimeter is required, describe how this is done.
 - e. General description of geometry of dosimeter and source; any material around dosimeter.
 - f. Description of environmental conditions during calibration.
 - g. Give the specified dose (rate) or exposure (rate); quantity and units of specified dose; how obtained.
 - h. Give material in which the dose (rate) was specified.
 - i. Give specified accuracy of the calibration.
2. Routine dosimetry
 - a. Personnel that perform day-to-day dosimetry measurements.
 - b. Give type of dosimeter(s) used.
 - c. If commercial equipment is used, give make and model.
 - d. For pulse-type radiation, are dosimeters or detectors used to monitor all irradiations.
 - e. If dosimeters are used in equilibrium material, specify material, thickness and geometry.
 - f. If calibration of dosimeters is required, describe how this is done.
 - g. Give units or quantities of the dose specified and in which material.
 - h. Observations on typical irradiation of the dosimeters: handling, environmental conditions, exposure to UV light, directional effects.
 - i. Describe location of dosimeters in the radiation field and in relation to the devices being tested.

- j. Observations on typical readings of the dosimeters; handling, TLD reader settings and behavior, length of time between exposure and readout.
 - k. Give reproducibility and accuracy of these routine measurements.
 - l. If TLDs are used, are they annealed and used repeatedly; anneal cycle; total number of times they are reused; total accumulated dose.
- E. General Comments from Facility Personnel
- 1. What do they feel are problem areas in their dosimetry measurements?
 - 2. What type of dosimetry standard would they like to see developed? What dosimetry system would be most useful to them?

DISTRIBUTION

Defense Communication Engineer Center
1860 Wiehle Avenue
Reston, VA 22090
ATTN R410 James W. McLean

Director
Defense Communications Agency
Washington, D.C. 20305
ATTN Code 930 Monte T. Burgett, Jr.

Defense Documentation Center
Cameron Station
Alexandria, VA 22314
ATTN TC (12 copies)

Director
Defense Nuclear Agency
Washington, D.C. 20305
ATTN STTL Tech Library (3 copies)
ATTN STVL
ATTN DDST
ATTN RAEV
ATTN RAEV Maj W. Adams (2 copies)

Dir of Defense Rsch & Engineering
Department of Defense
Washington, DC 20301
ATTN DD/S&SS

Commander
Field Command
Defense Nuclear Agency
Kirtland AFB, NM 87115
ATTN FCPR

Director
Interservice Nuclear Weapons School
Kirtland AFB, NM 87115
ATTN Document Control

Director
Joint Strat TGT Planning Staff JCS
Offutt AFB
Omaha, NB 68113
ATTN JLTW-2

DISTRIBUTION (Cont'd)

Chief
Livermore Division Fld Command DNA
Lawrence Livermore Laboratory
P.O. Box 808
Livermore, CA 94550
ATTN FCPRL

Project Manager
Army Tactical Data Systems
U.S. Army Electronics Command
Fort Monmouth, NJ 07703
ATTN Dwaine B. Huewe

Commander
BMD System Command
P.O. Box 1500
Huntsville, AL 35807
ATTN BDMSC-TEN Noah J. Hurst

Commander
Frankford Arsenal
Bridge and Tacony Streets
Philadelphia, PA 19137
ATTN SARFA-FCD Marvin Elnick

Commander
Harry Diamond Laboratories
2800 Powder Mill Road
Adelphi, Md. 20783
ATTN DRXDO-EM R. Bostak
ATTN DRXDO-RC Robert B. Oswald, Jr.
ATTN DRXDO-EM J.W. Beilfuss
ATTN DRXDO-EM Robert E. McCoskey
ATTN DRXDO-NP Francis N. Wimenitz
ATTN DRXDO-TR Edward E. Conrad
ATTN DRXDO-RB Joseph R. Miletta
ATTN DRXDO-TT Tech Lib
ATTN K.G. Kerris, Aurora

Commanding Officer
Night Vision Laboratory
U.S. Army Electronics Command
Fort Belvoir, VA 22060
ATTN Capt Allan S. Parker

DISTRIBUTION (Cont'd)

Commander
Picatinny Arsenal
Dover, NJ 07801
ATTN SMUPA-ND-D-E
ATTN SMUPA-ND-W

Commander
Redstone Scientific Information Ctr
U.S. Army Missile Command
Restone Arsenal, AL 35809
ATTN Chief, Documents (3 copies)

Secretary of the Army
Washington, D.C. 20310
ATTN ODUSA or Daniel Willard

Commander
TRASANA
White Sands Missile Range, NM 88002
ATTN ATAA-EAC Francis N. Winans

Chief
U.S. Army Communications Sys Agency
Fort Monmouth, NJ 07703
ATTN SCCM-AD-SV Library

Commander
U.S. Army Electronics Command
Fort Monmouth, NJ 07703
ATTN DRSEL-GG-TD W.R. Werk
ATTN DRSEL-TL-IR Edwin T. Hunter
ATTN DRSEL-PL-ENV Hans A. Bomke

Commander-in-Chief
U.S. Army Europe and Seventh Army
APO New York 09403
ATTN ODCSE-E AEAGE-PI

Commander
U.S. Army Materiel Dev & Readiness Cmd
5001 Eisenhower Avenue
Alexandria, VA 22333
ATTN DRCDE-D Lawrence Flynn

DISTRIBUTION (Cont'd)

Commander

U.S. Army Missile Command

Redstone Arsenal, AL 35809

ATTN DRCPM-PE-EA Wallace O. Wagner

ATTN DRCPM-LCEX Howard H. Henriksen

ATTN DRCPM-MDTI CAPT Joe A. Sims

ATTN DRSMI-RGD Vic Ruwe

ATTN AMSI-RGP Victor W. Ruwe

Commander

U.S. Army Mobility Equip R&D Ctr

Fort Belvoir, VA 22060

ATTN STSFB-MW John W. Bond, Jr.

ATTN AMSEL-NV-SD J.H. Carter

Chief

U.S. Army Nuc and Chemical Surety Gp

Bldg. 2073, North Area

Ft. Belvoir, VA 22060

ATTN MOSG-ND Maj Sidney W. Winslow

Commander

U.S. Army Nuclear Agency

Fort Bliss, TX 79916

ATTN ATCN-W LTC Leonard A. Sluga

Commander

U.S. Army Test and Evaluation Comd

Aberdeen Proving Ground, MD 21005

ATTN DRSTE-EL Richard I. Kolchin

ATTN DRSTE-NB Russell R. Galasso

Commander

White Sands Missile Range

White Sands Missile Range, NM 88002

ATTN STEWS-TE-NT Marvin P. Squires

ATTN STEWS-TE-NO Harold L. Wright

ATTN STEWS-TE-NO Major John L. Meason

Commander

Naval Electronic Systems Command

Naval Electronic Systems Cmd Hqs

Washington, D.C. 20360

ATTN CODE 50451

ATTN ELEX 05323 Cleveland F. Watkins

ATTN CODE 504511 Charles R. Suman

ATTN PME 117-21

ATTN CODE 5032 Charles W. Neill

DISTRIBUTION (Cont'd)

Director
Naval Research Laboratory
Washington, D.C. 20375
ATTN CODE 2627 Doris R. Folen
ATTN CODE 6601 E. Wolicki
ATTN CODE 5216 Harold L. Hughes
ATTN CODE 5210 John E. Davey

Commander
Naval Sea Systems Command
Navy Department
Washington, D.C. 20362
ATTN SEA-9931 Samuel A. Barham
ATTN SEA-9931 Riley B. Lane

Commander
Naval Surface Weapons Center
White Oak, Silver Spring, Md. 20910
ATTN CODE WX21 Tech Lib
ATTN CODE WA50 John H. Malloy
ATTN CODE 244
ATTN CODE 431 Edwin B. Dean
ATTN CODE WA501 Navy Nuc Prgms Off
ATTN CODE 431 Jed Sazama

Commander
Naval Weapons Center
China Lake, CA 93555
ATTN CODE 533 Tech Lib

Commanding Officer
Naval Weapons Support Center
Crane, IN 47522
ATTN CODE 7024 James Ramsey
ATTN CODE 70242 Joseph A. Munarin

Director
Strategic Systems Project Office
Navy Department
Washington, DC 20376
ATTN NSP-27331 Phil Spector
ATTN NSP-2342 Richard L. Coleman
ATTN NSP-230 David Gold
ATTN SP 2701 John W. Pitsenberger

AF Aero-Propulsion Laboratory, AFSC
Wright-Patterson AFB, OH 45433
ATTN POE-2 Joseph F. Wise

DISTRIBUTION (Cont'd)

AF Institute of Technology, AU
Wright-Patterson AFB, OH 45433
ATTN ENP Charles J. Bridgman

AF Materials Laboratory, AFSC
Wright-Patterson AFB, OH 45433
ATTN LTE

AF Weapons Laboratory, AFSC
Kirtland AFB, NM 87117
ATTN ELP TREE Section
ATTN ELA
ATTN SAS
ATTN ELP CAPT John G. Tucker
ATTN SAT
ATTN SAB
ATTN ELS Albert Matteucci

AFTAC
Patrick AFB, FL 32925
ATTN TFS Maj. Marion F. Schneider

Commander
ASD
WPAFB, OH 45433
ATTN ASD-YH-EX LTC Robert Leverette

Headquarters
Electronic Systems Division (AFSC)
Hanscom AFB, MA 01731
ATTN DCD/SATIN IV
ATTN YSEV
ATTN YWET

Commander
Foreign Technology Division, AFSC
Wright-Patterson AFB, OH 45433
ATTN ETET CAPT. Richard C. Husemann

Commander
Rome Air Development Center, AFSC
Griffiss AFB, NY 13440
ATTN RBRAC I.L. Krulac
ATTN RBRP Jack S. Smith

DISTRIBUTION (Cont'd)

SAMSO/DY
Post Office Box 92960
Worldway Postal Center
Los Angeles, CA 90009
ATTN DYS Maj. Larry A. Darda

SAMSO/IN
Post Office Box 92960
Worldway Postal Center
Los Angeles, CA 90009
ATTN IND I.J. Judy

SAMSO/MN
Norton AFB, CA 92409
ATTN MNNG Capt. David J. Strobel
ATTN MNNG
ATTN MNNH

SAMSO/RS
Post Office Box 92960
Worldway Postal Center
Los Angeles, CA 90009
ATTN RSSE LTC Kenneth L. Gilbert

SAMSO/SK
Post Office Box 92960
Worldway Postal Center
Los Angeles, CA 90009
ATTN SKF Peter H. Stadler

Commander in Chief
Strategic Air Command
Offutt AFB, NB 68113
ATTN XPFS Maj. Brian G. Stephan
ATTN NRI-STINFO Library

University of California
Lawrence Livermore Laboratory
P.O. Box 808
Livermore, CA 94550
ATTN Tech Info Dept L-3
ATTN Lawrence Cleland L-156
ATTN Hans Kruger L-96
ATTN Joseph E. Keller, Jr. L-125

Los Alamos Scientific Laboratory
P.O. Box 1663
Los Alamos, NM 87545
ATTN Doc. Cont. for J. Arthur Freed

DISTRIBUTION (Cont'd)

Sandia Laboratories
P.O. Box 5800
Albuquerque, NM 87115
ATTN DOC CON for 3141 Sandia Rpt Coll
ATTN DOC CON for Org 2110 J.A. Hood
ATTN DOC CON for Org 1933 F.N. Coppage
ATTN G.J. Lockwood 5232
ATTN William Buckalew
ATTN Lawrence Posey

Department of Commerce
National Bureau of Standards
Washington, D.C. 20234
ATTN Judson C. French, A357 Tech
ATTN W.M. Bullis, A355 Tech

Aerojet Electro-Systems Co Div
Aerojet-General Corp
P.O. Box 296
Azusa, CA 91702
ATTN Thomas D. Hanscome

Aeronutronic, Ford Corp
Aerospace & Communications Ops
Aeronutronic Div
Ford & Jamboree Roads
Newport Beach, CA 92663
ATTN Tech Info Section
ATTN Ken C. Attinger

Aeronutronic, Ford Corp
Western Development Laboratories Div
3939 Fabian Way
Palo Alto, CA 94303
ATTN Samuel R. Crawford MS 531

Aerospace Corp
P.O. Box 92957
Los Angeles, CA 90009
ATTN Irving M. Garfunkel
ATTN J. Benveniste
ATTN Julian Reinheimer
ATTN S. P. Bower

AVCO Research & Systems Group
201 Lowell Street
Wilmington, MA 01887
ATTN Research Lib A830, Rm 7201

DISTRIBUTION (Cont'd)

The BDM Corp
1920 Aline Ave
Vienna, VA 22180
ATTN T.H. Neighbors

The Bendix Corp
Communication Division
East Joppa Road - Towson
Baltimore, MD 21204
ATTN Document Control

The Bendix Corp
Research Laboratories Div
Bendix Center
Southfield, MI 48076
ATTN Max Frank
ATTN Mgr Prgm Dev Donald J. Niehaus

The Bendix Corp
Navigation and Control Div
Teterboro, NJ 07608
ATTN George Gartner

The Boeing Company
P.O. Box 3707
Seattle, WA 98124
ATTN David L. Dye MS 87-75
ATTN Aerospace Library
ATTN Howard W. Wicklein MS 17-11
ATTN Robert S. Caldwell 2R-00
ATTN Roger L. Guay BREL MS 2R-00

Booz-Allen and Hamilton, Inc.
106 Apple Street
New Shrewsbury, NJ 07724
ATTN Raymond J. Chrisner

California Inst. of Tech.
Jet Propulsion Lab
4800 Oak Park Grove
Pasadena, CA 91103
ATTN J. Bryden
ATTN A.G. Stanley
ATTN W.E. Price

Charles Stark Draper Laboratory, Inc.
68 Albany Street
Cambridge, MA 02139
ATTN Kenneth Fertig

DISTRIBUTION (Cont'd)

Computer Sciences Corp
201 LA Veta Drive N.E.
Albuquerque, NM 87108
ATTN Richard H. Dickhaut

Cutler-Hammer, Inc.
AIL Div
Comac Road
Deer Park, NY 11729
ATTN Central Tech Files Anne Anthony

The Dikewood Corp
1009 Bradbury Drive, S.E.
University Research Park
Albuquerque, NM 87106
ATTN L. Wayne Davis

E-Systems, Inc.
Greenville Div
P.O. Box 1056
Greenville, TX 75401
ATTN Library 8-50100

Effects Technology, Inc.
5383 Hollister Avenue
Santa Barbara, CA 93111
ATTN Edward John Steele

Fairfield Camera and Instrument Corp
464 Ellis Street
Mountain View, CA 94040
ATTN Sec Dept for 2-233 David K. Myers

Fairchild Industries, Inc.
Sherman Fairchild Technology Ctr
20301 Century Boulevard
Germantown, MD 20767
ATTN Mgr Config Data & Standards

Garrett Corp
P.O. Box 92248
Los Angeles, CA 90009
ATTN Robert E. Weir Dept 93-9

General Dynamics Corp
Electronics Div Orlando Operations
P.O. Box 2566
Orlando, FL 32802
ATTN D.W. Coleman

DISTRIBUTION (Cont'd)

General Electric Company
Space Division
Valley Forge Space Center
Goddard Blvd King of Prussia
P.O. Box 8555
Philadelphia, PA 19101
ATTN Larry I. Chasen
ATTN John L. Andrews
ATTN Joseph C. Peden VFSC, Rm 4230M

General Electric Company
Re-entry & Environmental Systems Div
P.O. Box 7722
3198 Chestnut Street
Philadelphia, PA 19101
ATTN John W. Palchefskey Jr
ATTN Robert V. Benedict

General Electric Company
Ordnance Systems
100 Plastics Avenue
Pittsfield, MA 01201
ATTN Joseph J. Reidl

General Electric Company
Tempo-Center for Advanced Studies
816 State Street (P.O. Drwr QQ)
Santa Barbara, CA 93102
ATTN M. Espig
ATTN DASIAC
ATTN Royden R. Rutherford

General Electric Company
P.O. Box 1122
Syracuse, NY 13201
ATTN CSP 0-7 L.H. Dee

General Electric Company
Aircraft Engine Group
Evendale Plant
Cincinnati, OH 45215
ATTN John A. Ellerhorst E 2

General Electric Company
Aerospace Electronics Systems
French Road
Utica, NY 13503
ATTN W.J. Patterson Drop 233
ATTN Charles M. Hewison Drop 624

DISTRIBUTION (Cont'd)

General Electric Company-Tempo
ATTN: DASIAC
C/O Defense Nuclear Agency
Washington, D.C. 20305
ATTN William Alfonte

Georgia Institute of Technology
Georgia Tech Research Inst
Atlanta, GA 30332
ATTN R. Curry

Grumman Aerospace Corp
South Oyster Bay Road
Bethpage, NY 11714
ATTN Jerry Rogers Dept 533

GTE Sylvania, Inc.
Electronics Systems Grp-Eastern Div
77 A Street
Needham, MA 02194
ATTN James A. Waldon
ATTN Charles A. Thornhill Librarian
ATTN Leonard L. Blaisdell

GTE Sylvania, Inc.
189 B Street
Needham Heights, MA 02194
ATTN H & V Group Mario A. Nurefora
ATTN Herbert A. Ullman

Gulton Industries, Inc.
Engineered Magnetics Division
13041 Cerise Avenue
Hawthorne, CA 90250
ATTN Engnmagnetics Div

Harris Corp
Harris Semiconductor Div
P.O. Box 883
Melbourne, FL 32901
ATTN Wayne E. Abare MS 16-111
ATTN Carl F. Davis MS 17-220
ATTN T.L. Clark MS 4040

DISTRIBUTION (Cont'd)

Hazeltine Corp
Pulaski Road
Green Lawn, NY 11740
ATTN Tech Info Ctr M. Waite

Honeywell Inc
Government and Aeronautical
Products Division
2600 Ridgeway Parkway
Minneapolis, MN 55413
ATTN Ronald R. Johnson A1622

Honeywell Inc
Aerospace Division
13350 U.S. Highway 19
St. Petersburg, FL 33733
ATTN M.S. 725-J Stacey H. Graff
ATTN Harrison H. Noble M.S. 725-5A

Honeywell Inc
Radiation Center
2 Forbes Road
Lexington, MA 02173
ATTN Technical Library

Hughes Aircraft Company
Centinela and Teale
Culver City, CA 90230
ATTN John B. Singletary MS 6-D133
ATTN Billy W. Campbell MS 6-E-110
ATTN Kenneth R. Walker MS D157

Hughes Aircraft Company
Space Systems Div
P.O. Box 92919
Los Angeles, CA 90009
ATTN Edward C. Smith MS A620
ATTN William W. Scott MS A1080

IBM Corp
Route 17C
Owego, NY 13827
ATTN Frank Frankovsky

IIT Research Institute
10 West 35th Street
Chicago, IL 60616
ATTN Irving N. Mindel

DISTRIBUTION (Cont'd)

Intl Tel & Telegraph Corp
500 Washington Avenue
Nutley, NJ 07110
ATTN Alexander T. Richardson

IRT Corp
P.O. Box 80817
San Diego, CA 92138
ATTN R.L. Mertz
ATTN Ralph H. Stahl
ATTN Leo D. Cotter
ATTN MDC
ATTN John W. Harrity
ATTN J.L. Azarewicz

JAYCOR
205 S. Whiting Street, Suite 500
Alexandria, VA 22304
ATTN Robert Sullivan
ATTN Catherine Turesko

John Hopkins University
Applied Physics Laboratory
Johns Hopkins Road
Laurel, MD 20810
ATTN Peter E. Partridge

Kaman Sciences Corp
P.O. Box 7463
Colorado Springs, CO 80933
ATTN Albert P. Bridges
ATTN Donald H. Bryce

Litton Systems, Inc.
Guidance & Control Systems Div
5500 Canoga Avenue
Woodland Hills, CA 91364
ATTN Val J. Ashby MS 67
ATTN John P. Retzler

Lockheed Missiles & Space Co., Inc.
P.O. Box 504
Sunnyvale, CA 94088
ATTN Benjamin T. Kimura Dept 81-14
ATTN Edwin A. Smith Dept 85-85
ATTN Dept 81-01 G.H. Morris
ATTN L. Rossi Dept 81-64
ATTN Dept 85-85 Samuel I. Taimuty

DISTRIBUTION (Cont'd)

Lockheed Missiles and Space Company
3251 Hanover Street
Palo Alto, CA 94304
ATTN Tech Info Ctr D/Col1

LTV Aerospace Corp
Vought Systems Division
P.O. Box 6267
Dallas, TX 75222
ATTN Technical Data Center

LTV Aerospace Corp
Michigan Division
P.O. Box 909
Warren, MI 48090
ATTN Tech Lib

M.I.T. Lincoln Laboratory
P.O. Box 73
Lexington, MA 02173
ATTN Leona Loughlin Librarian A-082

Martin Marietta Aerospace
Orlando Division
P.O. Box 5837
Orlando, FL 32805
ATTN Mona C. Griffith Lib MP-30
ATTN Jack M. Ashford MP-537
ATTN William W. Mras MP-413

McDonnell Douglas Corp
Post Office Box 516
St. Louis, Missouri 63166
ATTN Tech Lib
ATTN Tom Ender

Mission Research Corp
735 State Street
Santa Barbara, CA 93101
ATTN William C. Hart

Mission Research Corp-San Diego
7650 Convoy Court
San Diego, CA 92111
ATTN V.A.J. Van Lint

DISTRIBUTION (Con't)

National Academy of Sciences
ATTN: National Materials Advisory Board
2101 Constitution Avenue
Washington, D.C. 20418
ATTN R.S. Shane Nat Materials Advsy

Northrop Corp
Electronic Div
1 Research Park
Palos Verdes Peninsula, CA 90274
ATTN Vincent R. Demartino
ATTN Boyce T. Ahlport

Northrop Corp
Northrop Research and Technology Ctr
3401 West Broadway
Hawthorne, CA 90250
ATTN Orlie L. Curtis, Jr.
ATTN J.R. Srouer
ATTN David N. Pocock
ATTN L.T. Smith A-3144/60

Palisades Inst. for Rsch Services Inc.
201 Varick Street
New York, NY 10014
ATTN Records Supervisor

Power Physics Corp
542 Industrial Way West
P.O. Box 626
Eatontown, NJ 07724
ATTN Mitchell Baker

R & D Associates
P.O. Box 9695
Marina Del Rey, CA 90291
ATTN S. Clay Rogers

Raytheon Company
Hartwell Road
Bedford, MA 01730
ATTN Gajanan H. Joshi Radar Sys Lab

Raytheon Company
528 Boston Post Road
Sudbury, MA 01776
ATTN Harold L. Flescher

DISTRIBUTION (Cont'd)

RCA Corporation
Government & Commercial Systems
ASTRO Electronics Div
P.O. Box 800, Locust Corner
Princeton, NJ 08540
attn George J. Brucker

RCA Corporation
David Sarnoff Research Ctr
W. Windsor Twp
201 Washington Road, P.O. Box 432
Princeton, NJ 08540
ATTN K.H. Zaininger

RCA Corporation
Camden Complex
Front & Cooper Sts
Camden, NJ 08012
ATTN E. Van Keuren 13-5-2

Research Triangle Inst
P.O. Box 12194
Research Triangle Park, NC 27709
ATTN Eng Div Mayrant Simons Jr.

Rockwell International Corp
3370 Miraloma Ave
Anaheim, CA 92803
ATTN N.J. Rudie FA53
ATTN James E. Bell HA10
ATTN George C. Messenger FB61
ATTN K.F. Hull
ATTN L. Apodaca FA53
ATTN Virgil Strahan

Rockwell International Corporation
5701 West Imperial Highway
Los Angeles, CA 90009
ATTN T.B. Yates

Rockwell International Corporation
Electronics Operations
Collins Radio Group
5225 C Avenue NE
Cedar Rapids, IA 52406
ATTN Alan A. Langenfeld
ATTN Dennis Sutherland
ATTN Mildred A. Blair

DISTRIBUTION (Cont'd)

Sanders Associates, Inc.
95 Canal Street
Nashua, NH 03060
ATTN Moe L. Aitel NCA 1-3236

Science Applications, Inc.
P.O. Box 2351
La Jolla, CA 92038
ATTN Larry Scott
attn J. Robert Beyster

Simulation Physics, Inc.
41 "B" Street
Burlington, MA 01803
ATTN Roger G. Little

The Singer Company (Data Systems)
150 Totowa Road
Wayne, NJ 07470
ATTN Tech Info Ctr

Sperry Flight Systems Div
Sperry Rand Corp
P.O. Box 21111
Phoenix, AZ 85036
ATTN D. Andrew Schow

Sperry Rand Corp
Univac Div
Defense Systems Div
P.O. Box 3525 Mail Station 1931
St. Paul, MN 55101
ATTN James A. Inda MS 41T25

Sperry Rand Corp
Sperry Div
Sperry Gyroscope Div
Sperry Systems Management Div
Marcus Avenue
Great Neck, NY 11020
ATTN Paul Marraffino
ATTN Charles L. Craig EV

Stanford Research Inst
333 Ravenswood Ave
Menlo Park, CA 94025
ATTN Philip J. Dolan

DISTRIBUTION (Cont'd)

Sundstrand Corp
4751 Harrison Avenue
Rockford, IL 61101
ATTN Curtis B. White

Texas Instruments, Inc.
P.O. Box 6015
Dallas, TX 75222
ATTN Donald J. Manus MS 72

TRW Systems Group
One Space Park
Redondo Beach, CA 90278
ATTN H.H. Holloway R1-2036
ATTN Jerry I. Lubell R1-1144
ATTN John D. Nash, Bldg. 84
ATTN O.E. Adams R1-1144 (2 copies)
ATTN R.K. Plebuch R1-2078 (2 copies)
ATTN Tech Info Center/S-1930
ATTN Robert M. Webb R1-2410
ATTN William Beggs

TRW Systems Group
San Bernardino Operations
P.O. Box 1310
San Bernardino, CA 92402
ATTN F.B. Fay 527/710
ATTN Earl W. Allen

TRW Systems Group
P.O. Box 368
Clearfield, UT 84015
ATTN Donald W. Pugsley

United Technologies Corp
Hamilton Standard Div
Bradley International Airport
Windsor Locks, CT 06069
ATTN Raymond G. Giguere

Westinghouse Electric Corp
Defense and Electronic Systems Ctr
P.O. Box 1693
Friendship International Airport
Baltimore, MD 21203
ATTN Henry P. Kalapaca MS 3525

| | | | |
|--|---|--|------------------------------|
| U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET | 1. PUBLICATION OR REPORT NO. NBSIR 76-1135 | 2. Gov't Accession No. | 3. Recipient's Accession No. |
| 4. TITLE AND SUBTITLE RADIATION HARDNESS TESTING OF ELECTRONIC DEVICES: A SURVEY OF FACILITY DOSIMETRY PRACTICES | | 5. Publication Date September 1976 | |
| | | 6. Performing Organization Code 240.06 | |
| 7. AUTHOR(S) J. C. Humphreys and S.E. Chappell | | 8. Performing Organ. Report No. | |
| 9. PERFORMING ORGANIZATION NAME AND ADDRESS NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234 | | 10. Project/Task/Work Unit No. Z99QAXD072 & W.U. 05 | |
| | | 11. Contract/Grant No. | |
| 12. Sponsoring Organization Name and Complete Address (Street, City, State, ZIP) Director Defense Nuclear Agency Washington, D.C. 20305 Attn: RAEV, Captain R.R. Davis | | 13. Type of Report & Period Covered Final Jan - Sept 1976 | |
| | | 14. Sponsoring Agency Code | |
| 15. SUPPLEMENTARY NOTES | | | |
| 16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.) <p>As part of a program to develop better quality assurance in the measurement of total dose in the field of radiation-hardness testing of electronic devices, a survey was conducted at twelve radiation test facilities. The survey was carried out through personal visits at which time various characteristics of the test facilities and dosimetry procedures were noted. This report summarizes the results of the survey. Particular attention is given to the types of dosimetry problems perceived by the dosimetry personnel at the facilities as well as to general observations by the surveyor.</p> <p>The observations and information obtained through this survey led to some conclusions on where problems in total-dose measurements may occur. Some specific recommendations result and give direction to the program plan for developing more consistent measurement procedures within the radiation-hardness testing community.</p> | | | |
| 17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons) Dosimeter calibration; electronic devices; ionizing radiation; radiation dosimetry; radiation hardness testing; radiation sources; thermoluminescence dosimeters; total dose. | | | |
| 18. AVAILABILITY <input checked="" type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office Washington, D.C. 20402, SD Cat. No. C13 <input checked="" type="checkbox"/> Order From National Technical Information Service (NTIS) Springfield, Virginia 22151 | | 19. SECURITY CLASS (THIS REPORT) UNCLASSIFIED | 21. NO. OF PAGES 44 |
| | | 20. SECURITY CLASS (THIS PAGE) UNCLASSIFIED | 22. Price \$4.00 |

